

BIOMÉRIEUX

STOOL PREPROCESSING DEVICE

FOR MOLECULAR TESTING

The power of standardization...
in just 5 minutes



PIONEERING DIAGNOSTICS




STOOL PREPROCESSING DEVICE

**SPENDING TOO MUCH TIME PREPROCESSING STOOL?
YOU DON'T HAVE TO.**


Stool samples are among the most difficult and time-consuming clinical samples to process for molecular biology assays. This is now a thing of the past thanks to bioMérieux's new 4-step stool preprocessing device. It standardizes stool sample preparation for nucleic acid extraction of viruses, bacteria and parasites. And it only takes about 5 minutes.



Laboratory routine use

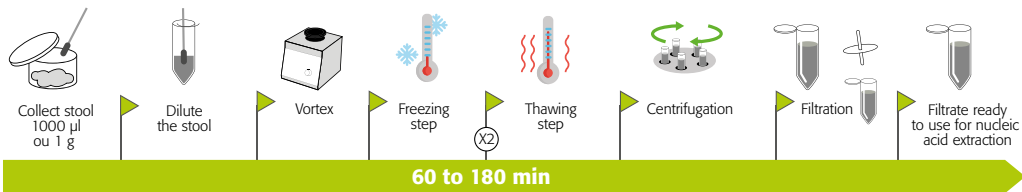

bioMérieux Stool Preprocessing Device use

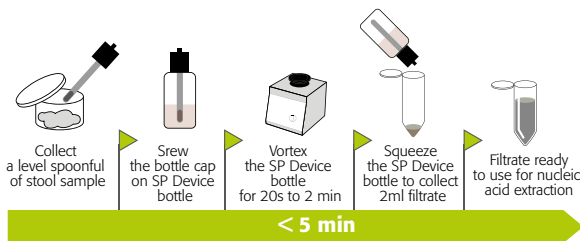

STANDARDIZE STOOL PREPROCESSING

- Calibration of the sampling
- Validated for qualitative and quantitative applications

SAVE HOURS - NOT MINUTES


- Just 5 minutes hands-on time
- Ready-to-use filtered solution for nucleic acids extraction

EXPERIENCE SIMPLICITY

- No sample weighing
- No pipetting

STOOL SECURE PROCESSING WORKFLOW

- Entirely closed process
- No sample contamination

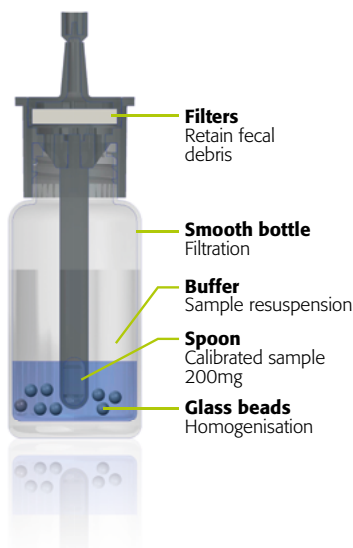

PRODUCT NAME	REFERENCE
Stool Preprocessing Device	Ref. 421061
Stool Preprocessing Device Vortex adapter	Ref. 422152
Stool Preprocessing Device Rack	Ref. 422163

Contact your local bioMérieux representative for availability